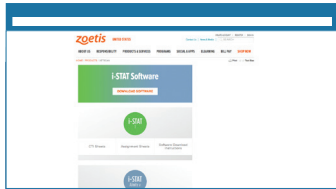## i-STAT
Alinity v

Installing OSi Software onto i-STAT Alinity v Using a USB Drive
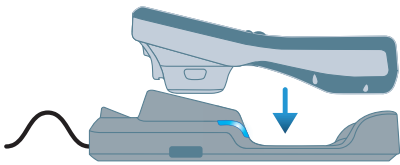
Go to:
www.zoetisUS.com/istatsoftware
> Select Download Software

Navigate to Download Your i-STAT Alinity v Handheld Analyzer Software

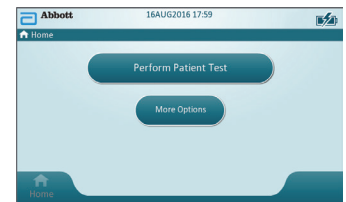> Select Downloadable i-STAT Alinity v OSiXX System Software

Save software to a USB drive

* Requires FAT32 formatted USB 2.0 memory stick

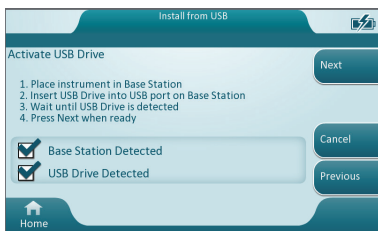** File must be saved on the top-level directory of the USB drive*

Place instrument into the Base Station and power on the instrument

Ensure Base Station is powered on.
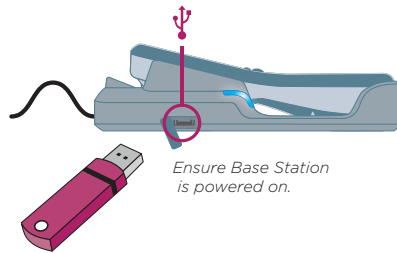
Insert USB drive into the USB port in the Base Station

Abbott   16AUG2016 17:59
Home
Perform Patient Test
More Options
Home

From the Home Screen:
> More Options
> Instrument Options
> Software Installation
> Install from USB

Install from USB
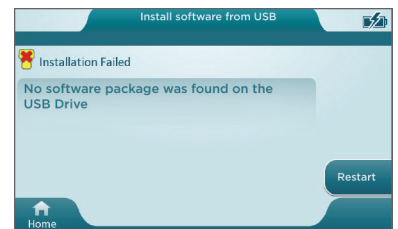
Activate USB Drive

1. Place instrument in Base Station
2. Insert USB Drive into USB port on Base Station
3. Wait until USB Drive is detected
4. Press Next when ready

☑ Base Station Detected
☑ USB Drive Detected

Next
Cancel
Previous
Home

Follow prompts until transfer is complete

SUCCESS

Alerts 1 of 1

New Software Installed
Quality Menu

An Electronic Simulator test is recommended.

Touch Quality Menu and then touch Perform Electronic Simulator Test to initiate an Electronic Simulator test.

Exit Alerts
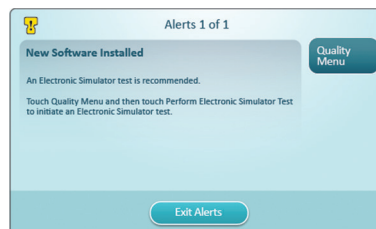
OSi Software Installation Results
SUCCESS

FAILURE

Install software from USB

☒ **Installation Failed**

No software package was found on the USB Drive

Restart
Home

OSi Software Installation Results
FAILURE

If additional assistance is required, please contact Zoetis Technical Support at 1-800-822-2947. Support is available 24 hours/day, 7 days/week.

zoetis